


Time Deviation  $\sigma_x(\tau)$

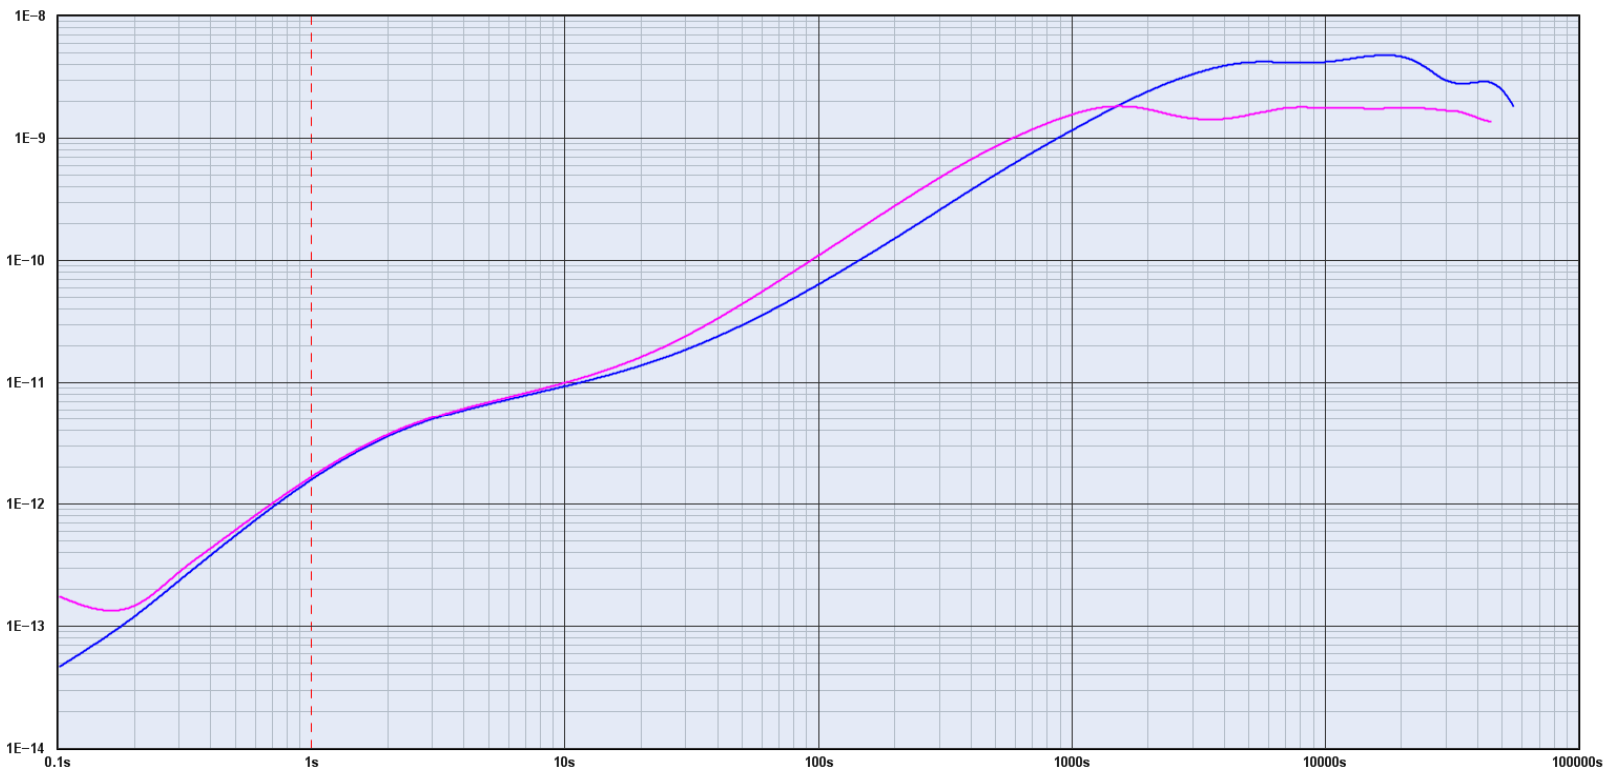

Trace	Notes	Input Freq	Sample Interval	TDEV at 1s	Duration	Acquired	Instrument
z3801		10 MHz	0.100 s	1.63E-12	3d 9h 50m 46s	2946457 pts	Symmetricom 3120A
z3810 vs Cs long		15 MHz	0.100 s	1.72E-12	2d 20h 51m 49s	2479086 pts	TimePod 5330A