


Allan Deviation $\sigma_y(\tau)$

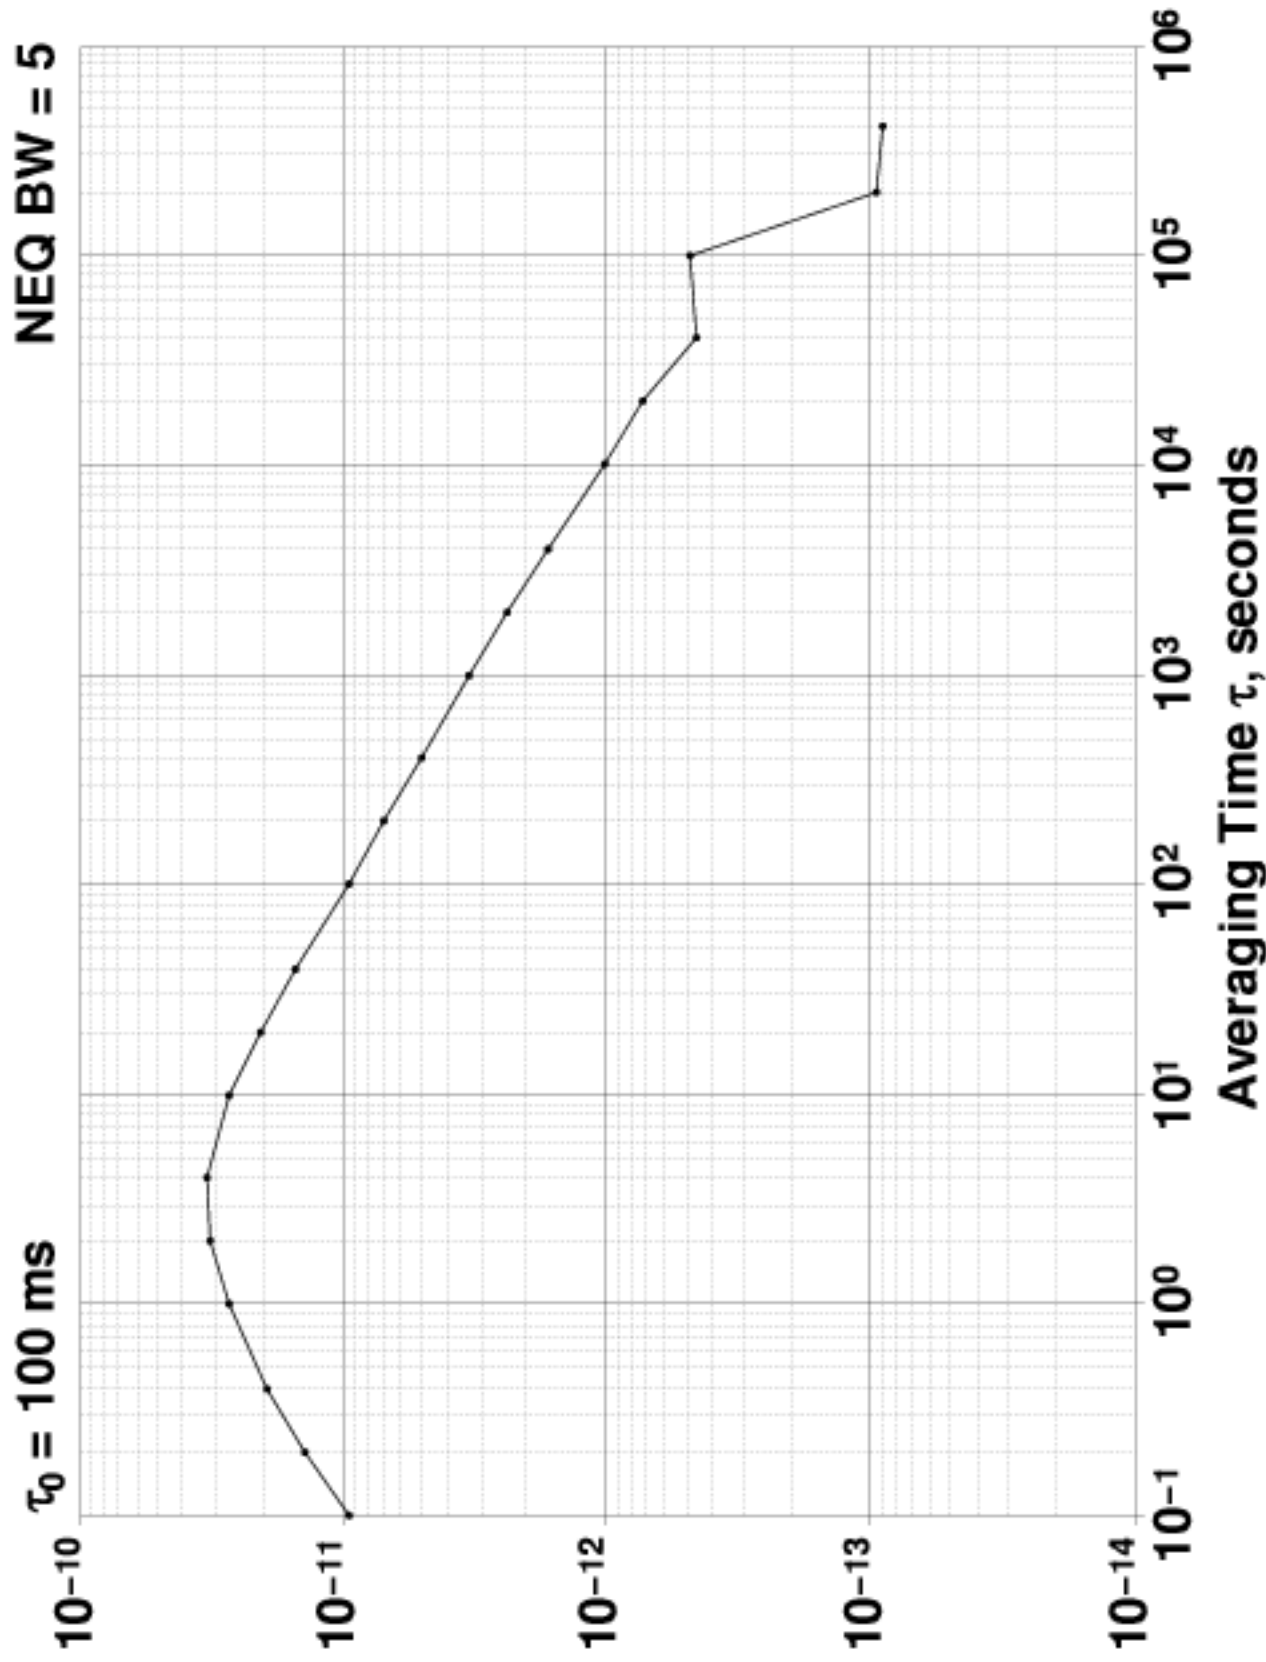


Allan Deviation $\sigma_y(\tau)$

$\tau_0 = 100 \text{ ms}$	Avg. Time (s)	Allan Deviation $\sigma_y(\tau)$	NEQ BW = 5
	0.1	9.3136×10^{-12}	
	0.2	1.3803×10^{-11}	
	0.4	1.9102×10^{-11}	
	1	2.6884×10^{-11}	
	2	3.1493×10^{-11}	
	4	3.225×10^{-11}	
	10	2.640×10^{-11}	
	20	2.013×10^{-11}	
	40	1.491×10^{-11}	
	100	9.53×10^{-12}	
	200	6.88×10^{-12}	
	400	5.03×10^{-12}	
	1000	3.35×10^{-12}	
	2000	2.38×10^{-12}	
	4000	1.65×10^{-12}	
	10000	1.02×10^{-12}	
	20000	7.2×10^{-13}	
	40000	4.5×10^{-13}	
	100000	4.9×10^{-13}	
	200000	9.6×10^{-14}	
	400000	9.0×10^{-14}	

Phase Difference

4.0x10⁻⁰⁹ s/div

Center: -5.227979x10⁻⁰⁵ s

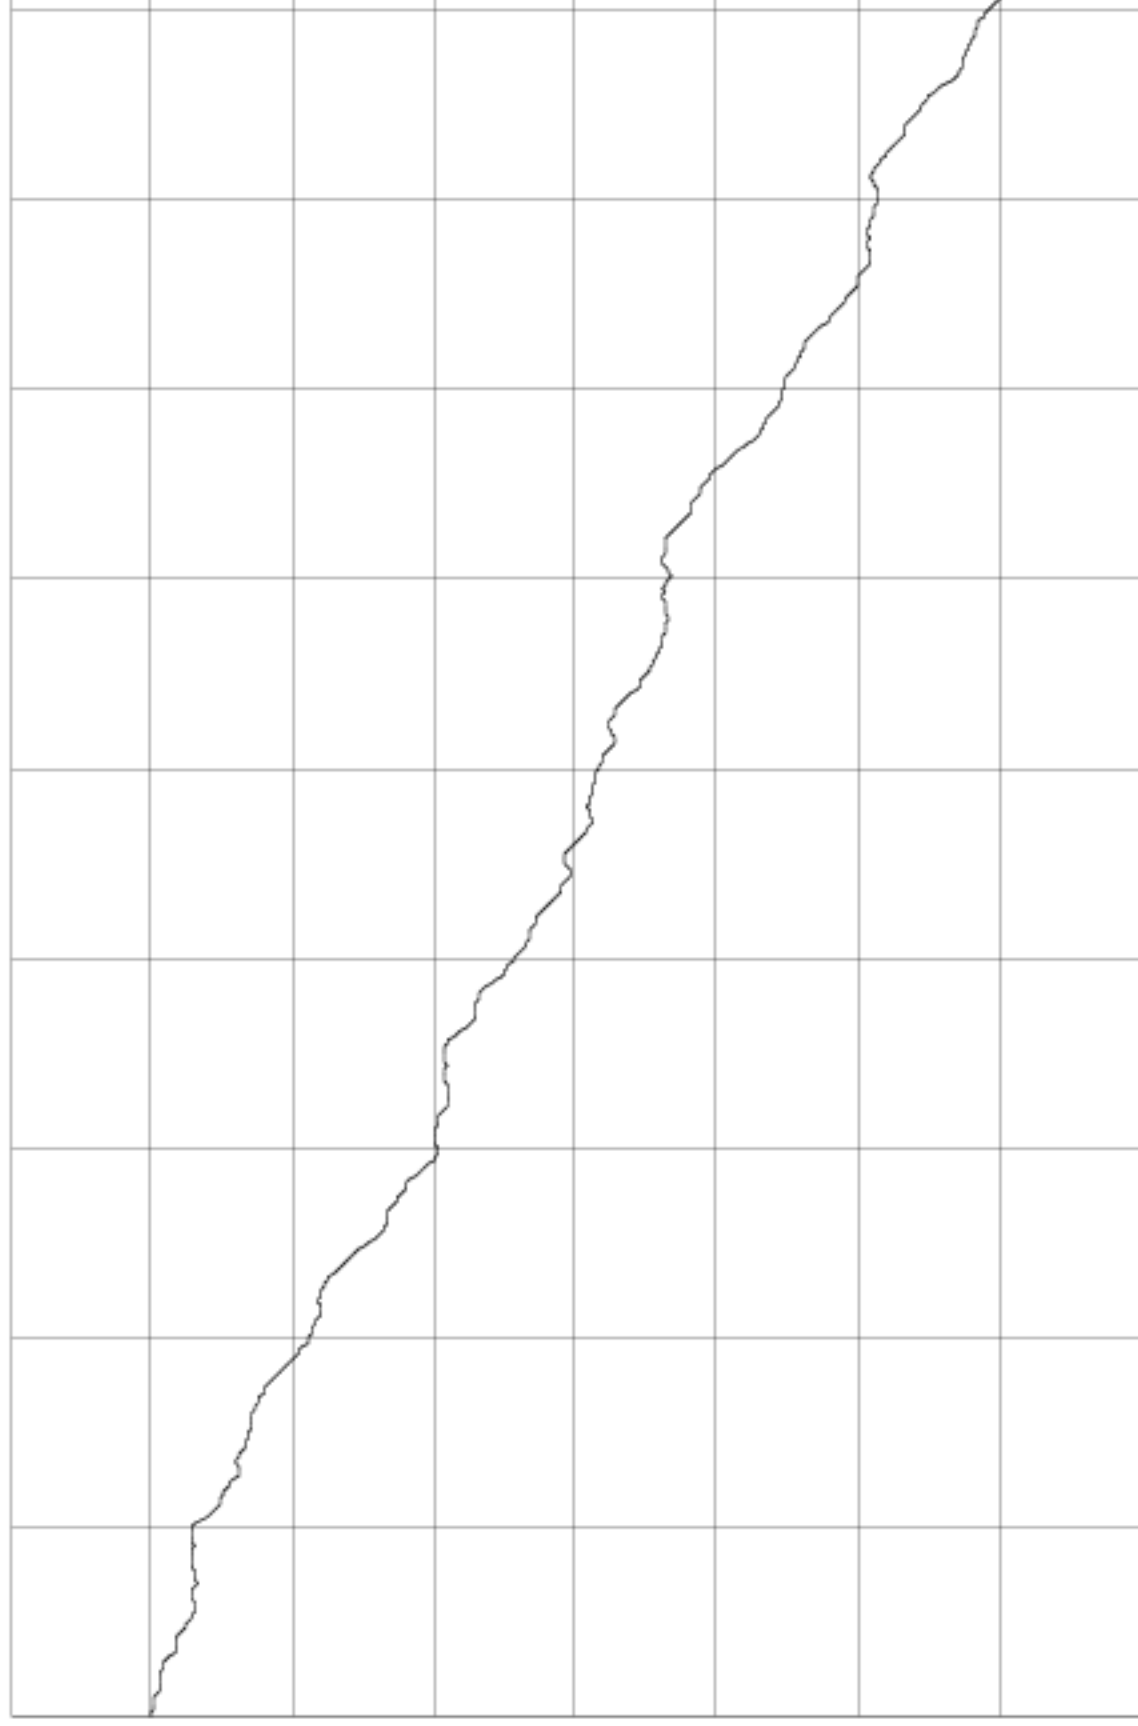

60s/div


Input 5.0 MHz 14 dBm

Reference 5.0 MHz 13 dBm

Frequency Difference

4.0×10^{-11} /div

Center: -5.060×10^{-11}

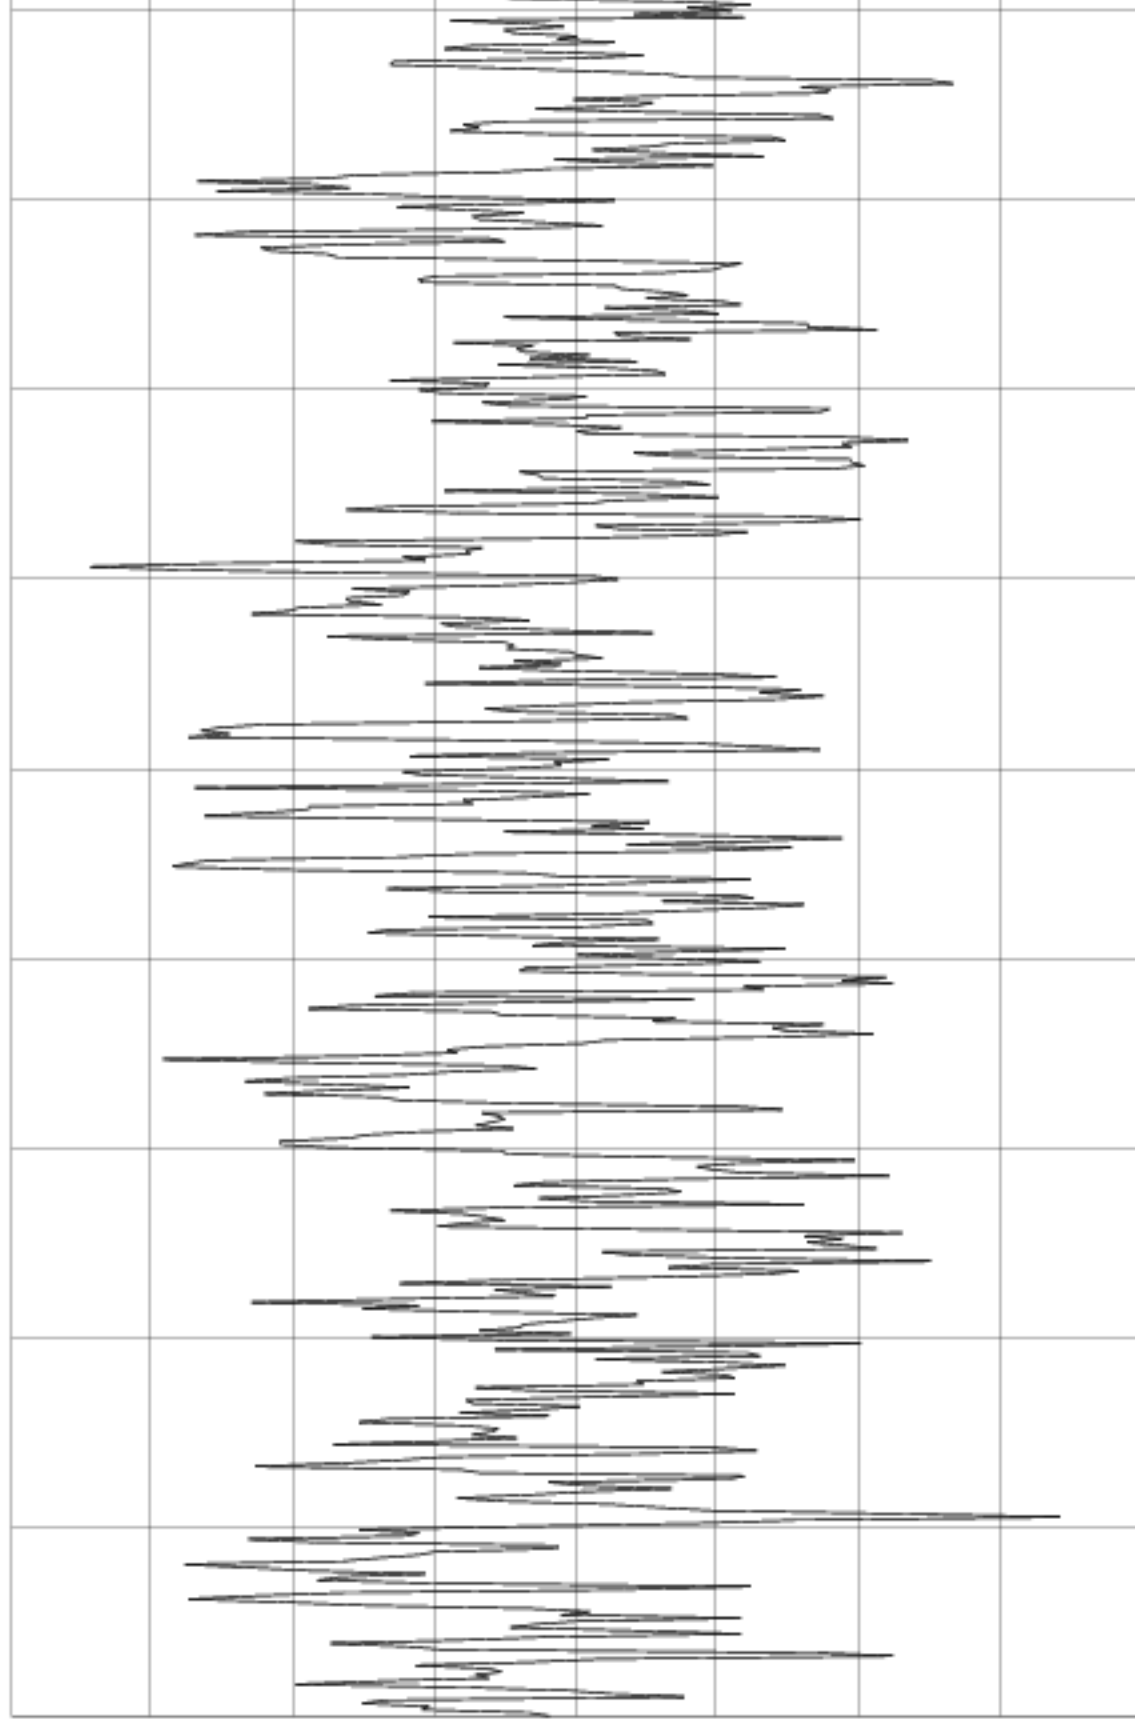

60s/div

Input 5.0 MHz 14 dBm

Reference 5.0 MHz 13 dBm


Frequency Counter

Sample Time (s)	Frequency (MHz)
1	4.99999999998682
10	5.00000000012958
100	5.000000000034644
1000	4.999999999974685

Reference Frequency: 5.0 MHz (auto)

$\mathcal{L}(f)$ Phase Noise at 5.0 MHz (dBc/Hz)

20 dB/Div

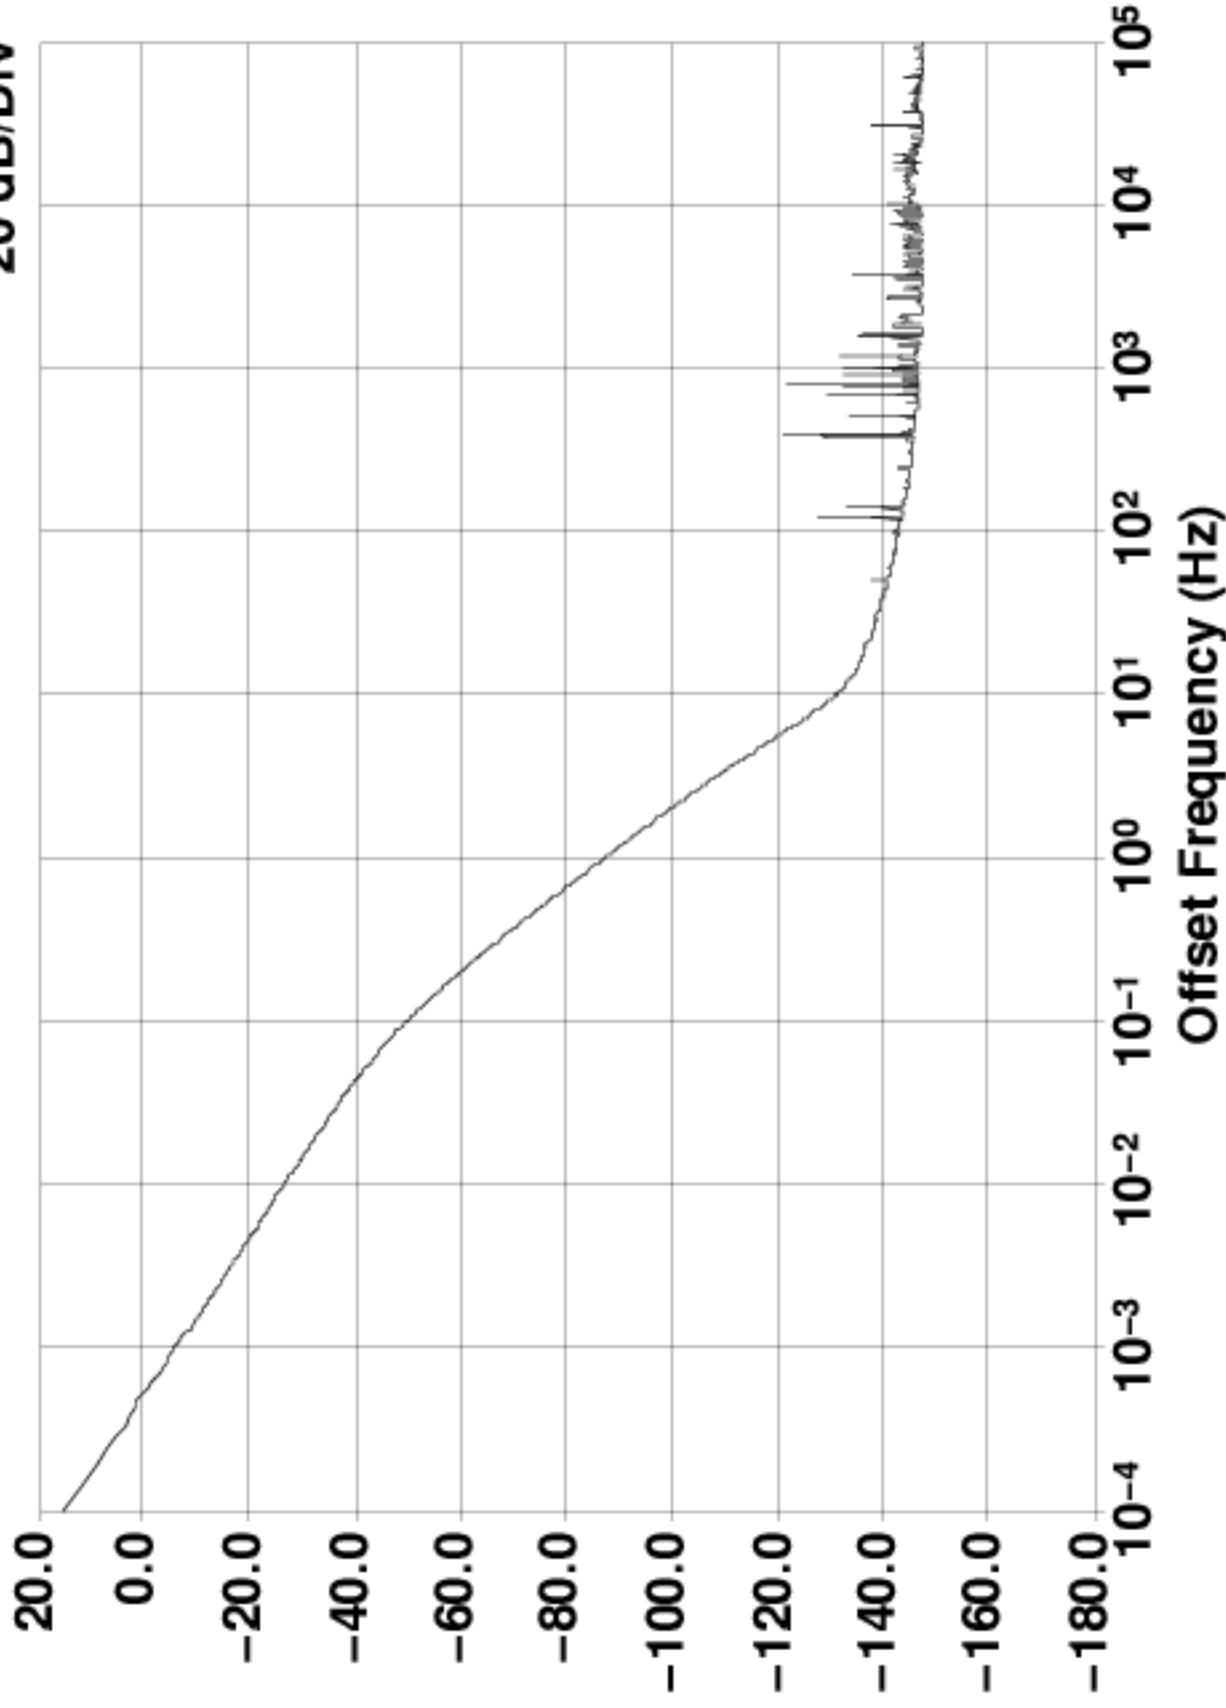

Input 5.0 MHz 14 dBm

Reference 5.0 MHz 13 dBm