

Allan Deviation $\sigma_y(\tau)$

$\tau_0 = 1 \text{ ms}$	Avg. Time (s)	Allan Deviation $\sigma_y(\tau)$	NEQ BW = 500
	0.001	1.8387×10^{-10}	
	0.002	9.2294×10^{-11}	
	0.004	4.7451×10^{-11}	
	0.01	2.0483×10^{-11}	
	0.02	1.2881×10^{-11}	
	0.04	1.0056×10^{-11}	
	0.1	8.609×10^{-12}	
	0.2	8.012×10^{-12}	
	0.4	7.609×10^{-12}	
	1	7.14×10^{-12}	
	2	6.92×10^{-12}	
	4	6.70×10^{-12}	
	10	6.97×10^{-12}	
	20	7.35×10^{-12}	
	40	7.72×10^{-12}	
	100	7.2×10^{-12}	
	200	7.0×10^{-12}	
	400	6.9×10^{-12}	
	1000	6.7×10^{-12}	
	2000	6.2×10^{-12}	
	4000	5.2×10^{-12}	


29/03/2007 20:39:20
2h 57m

TSC 5120A

Phase Difference

4.0×10^{-10} s/div

Center: 1.29446×10^{-07} s

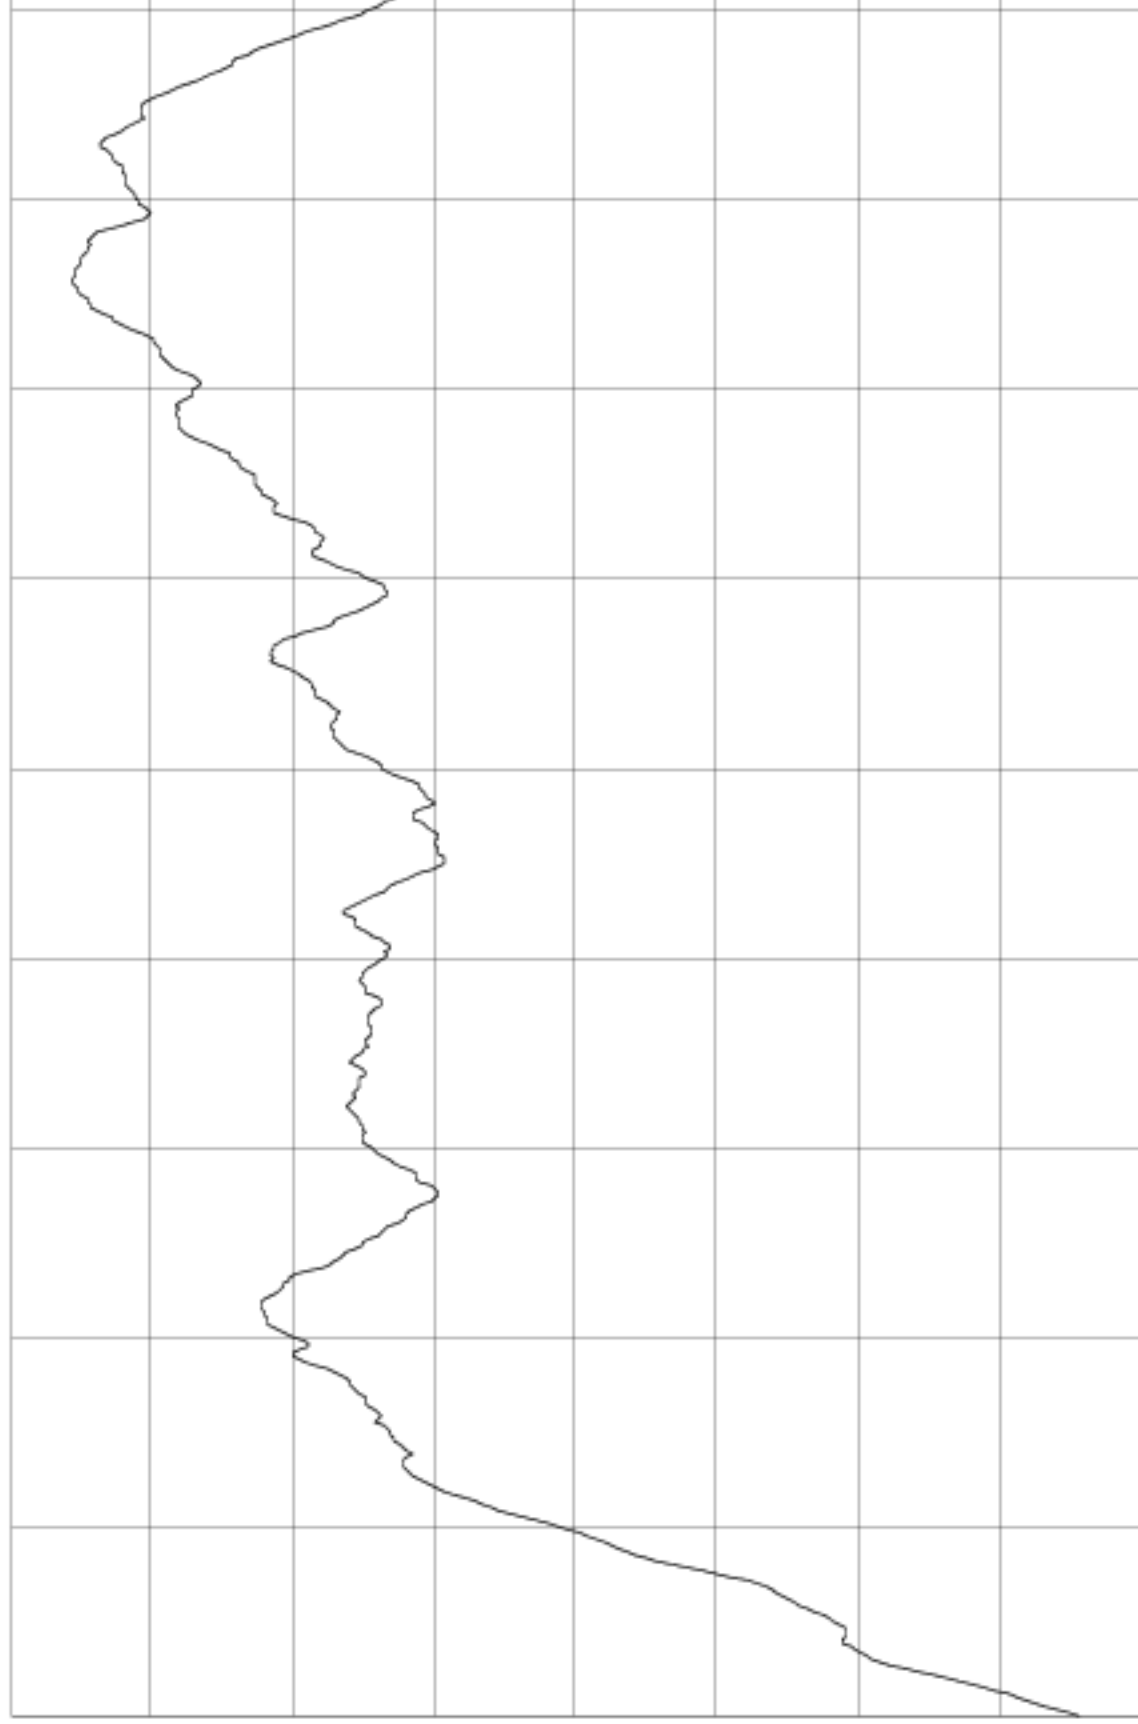

60s/div


Input 10.0 MHz 6 dBm

Reference 5.0 MHz 13 dBm

Frequency Difference

2.0×10^{-11} /div

Center: 3.095×10^{-12}

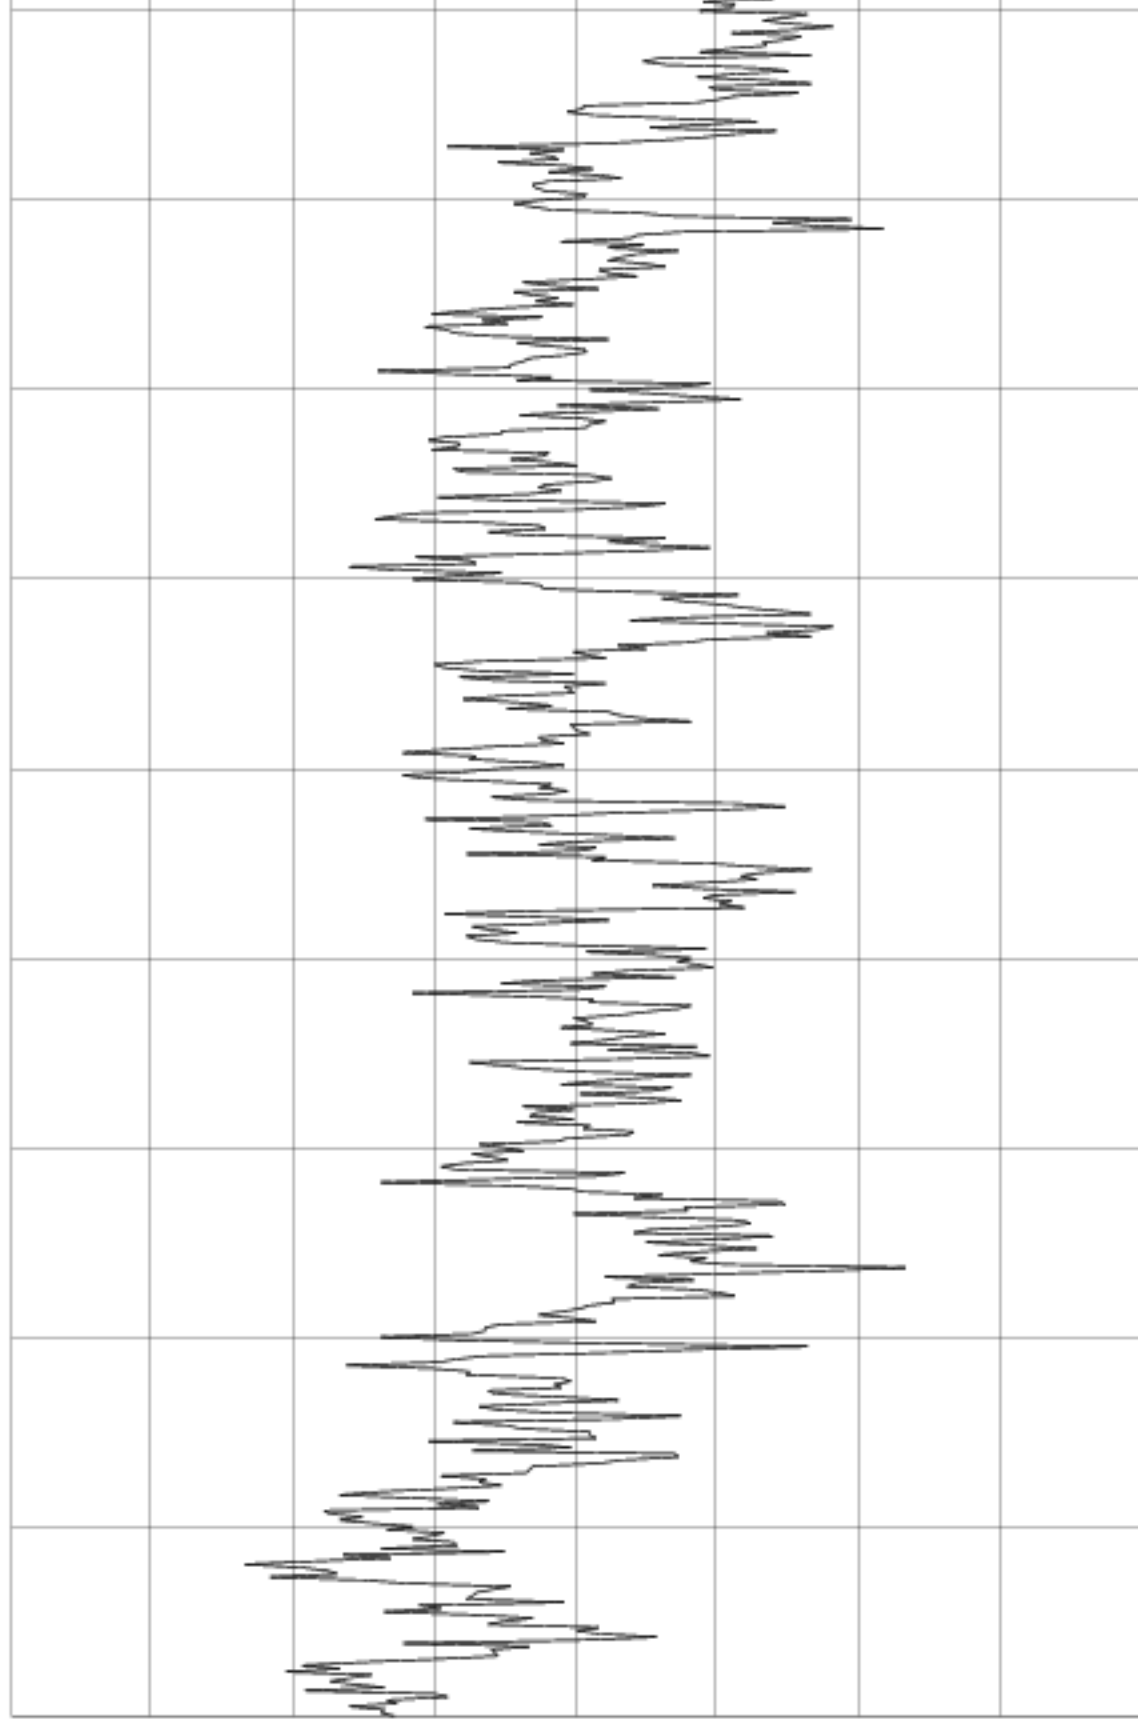

60s/div

Input 10.0 MHz 6 dBm

Reference 5.0 MHz 13 dBm


Frequency Counter

Sample Time (s)	Frequency (MHz)
1	9.9999999691334
10	9.99999996913306
100	9.999999969183794
1000	9.999999969033820

Reference Frequency: 5.0 MHz (auto)

$\mathcal{L}(f)$ Phase Noise at 10.0 MHz (dBc/Hz)

20 dB/Div

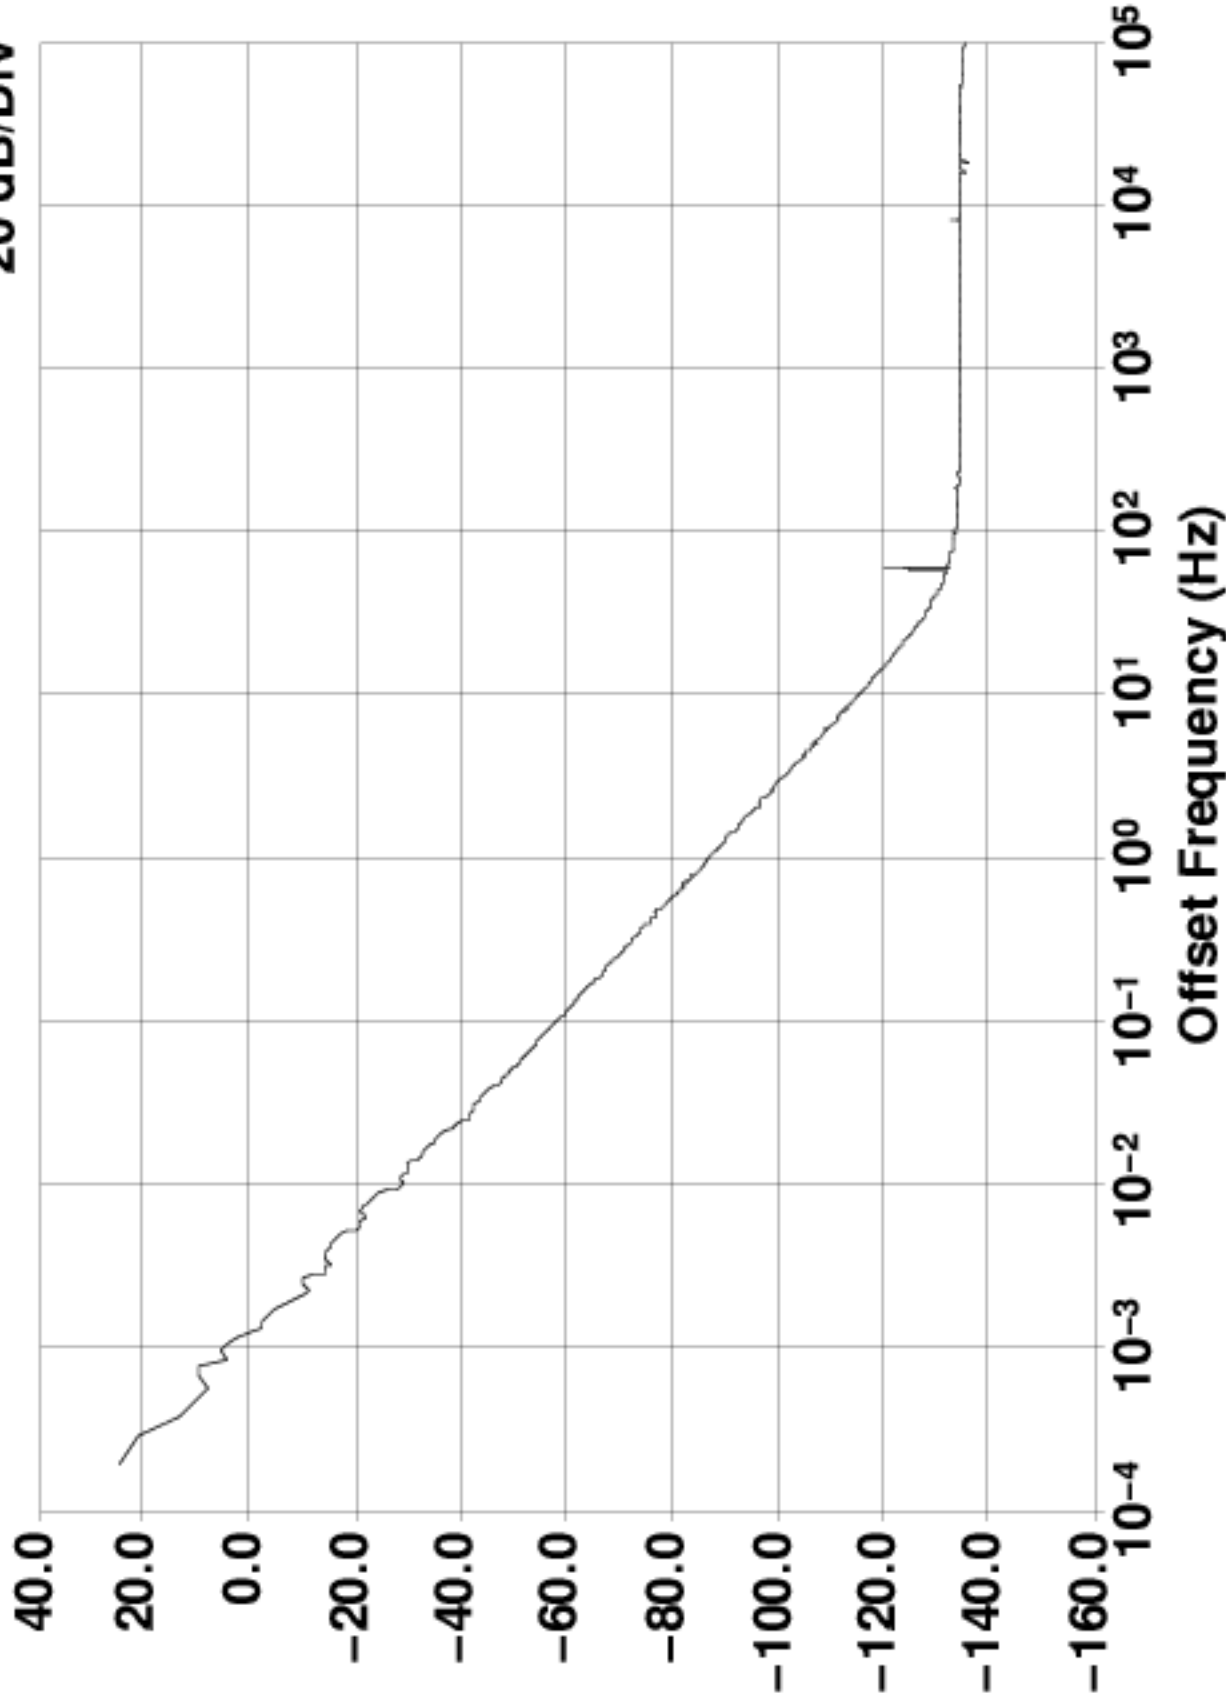

Input 10.0 MHz 6 dBm

Reference 5.0 MHz 13 dBm