


Phase Noise $\mathcal{L}(f)$ in dBc/Hz

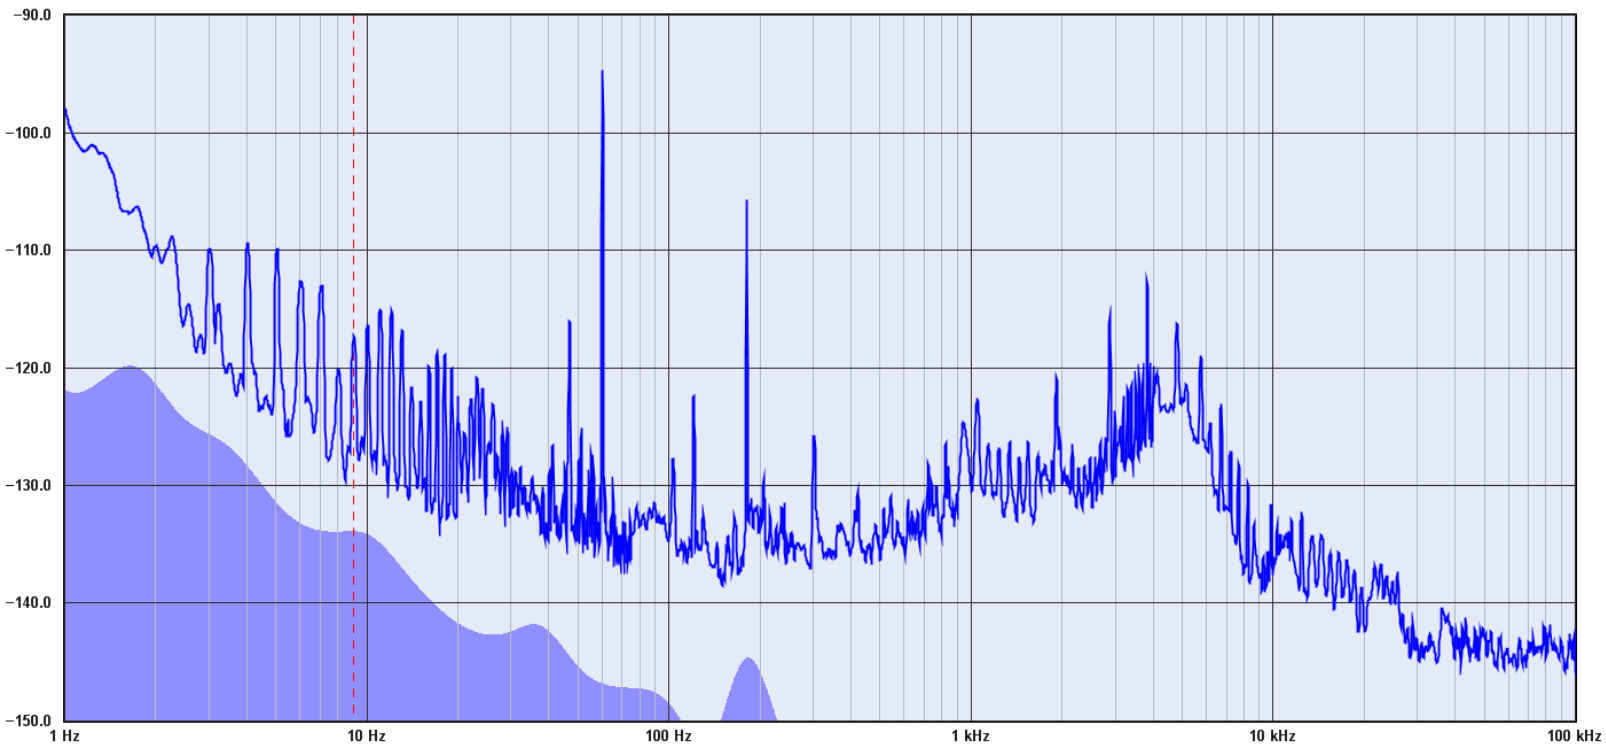

Trace	Notes	Input Freq	Sample Interval	dBc/Hz at 9 Hz	Duration	Acquired	Instrument
10 MHz vs ULN		10.000 MHz	0.010 s	-117.8	7m 9s	42853 pts	TimePod 5330A