


Frequency Difference (Zero-based)

Averaging window: 5 seconds

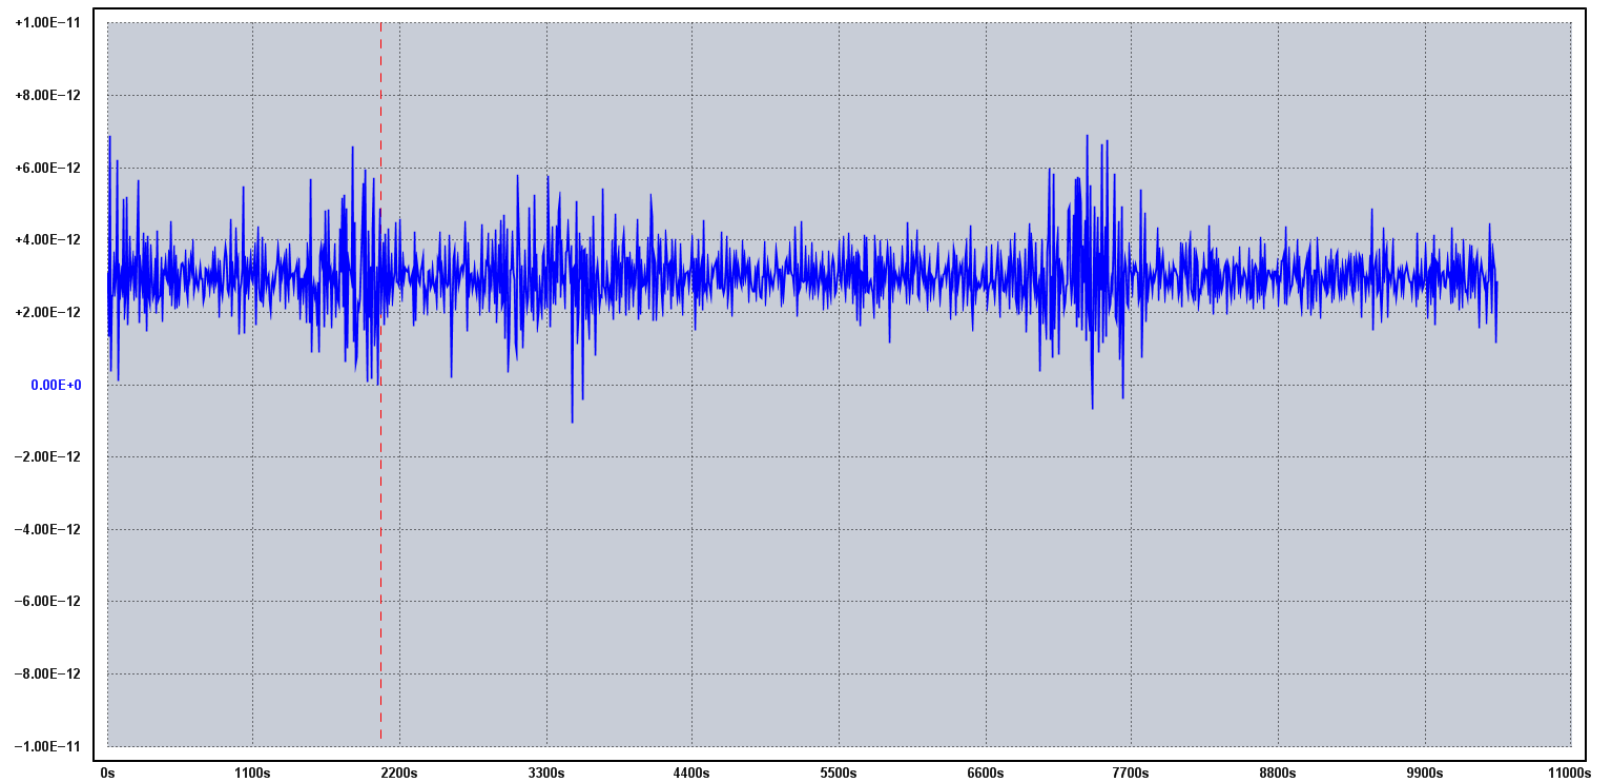

Trace	Notes	Input Freq	Sample Interval	Freq at 2050s	Duration	Acquired	Instrument
z3810 10m vs 15 m		15 MHz	0.100 s	15 000 000 Hz	2h 54m 8s	104480 pts	TimePod 5330A