


Original Phase Difference (Zero-based)

Averaging window: 5 seconds

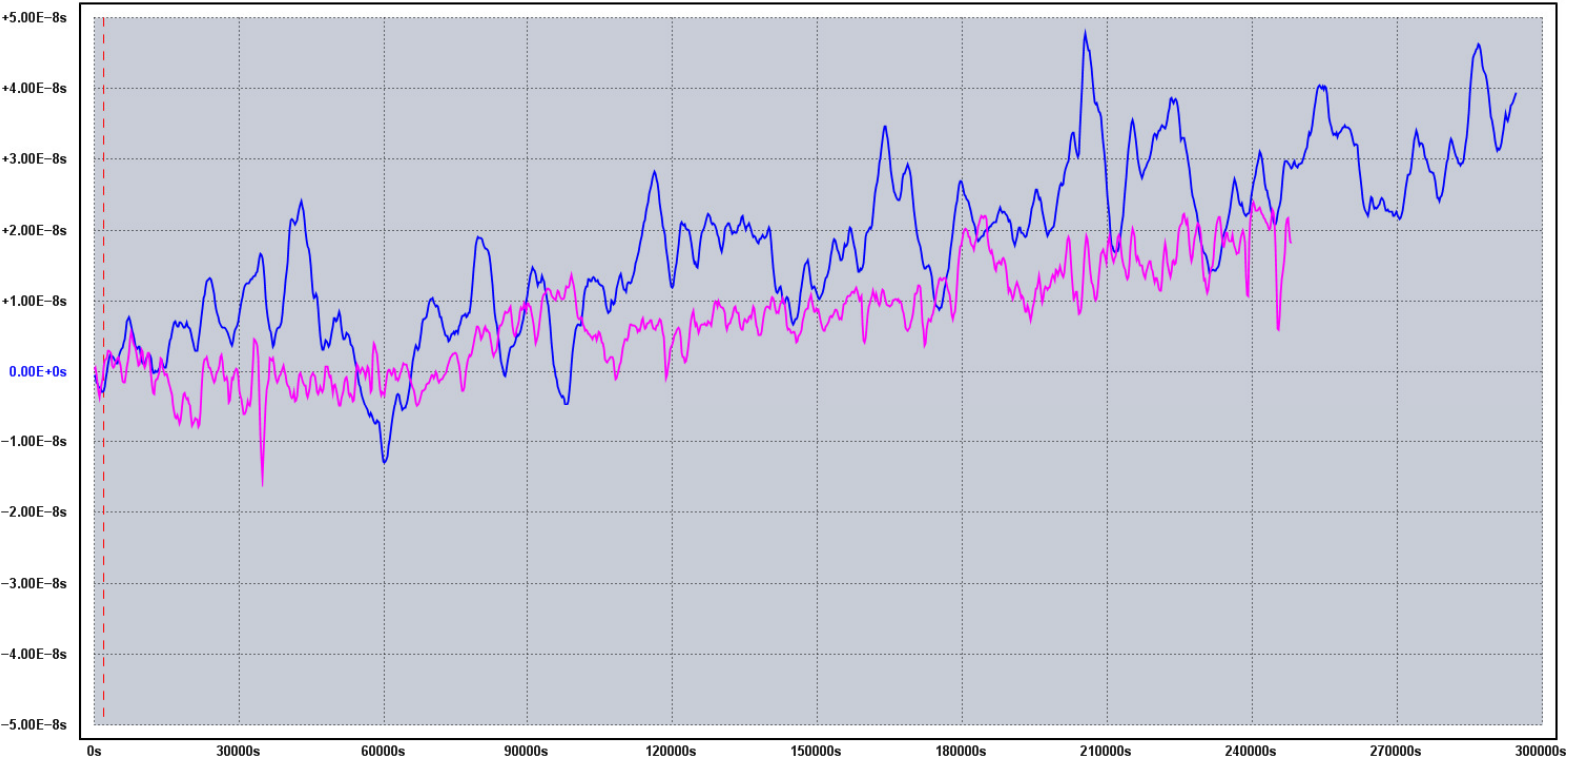

Trace	Notes	Input Freq	Sample Interval	Phase at 2050s	Duration	Acquired	Instrument
z3801		10 MHz	0.100 s	-2.77E-9s	3d 9h 50m 46s	2946457 pts	Symmetricom 3120A
z3810 vs Cs long		15 MHz	0.100 s	6.50E-10s	2d 20h 51m 49s	2479086 pts	TimePod 5330A